

VTxx/P SENSOR

INSTALLATION GUIDE:

BACK THE LOCK NUT UP TOWARDS THE AMPLIFIER HOUSING. SCREW IN THE SENSOR BY HAND UNTIL IT TOUCHES BOTTOM, THEN BACK OFF 1/4 TURN AND TIGHTEN THE LOCK NUT.

TECHNICAL DATA:




SUPPLY VOLTAGE...+7-29VDC
SUPPLY CURRENT....

MAX FLUID TEMPERATURE:

+248°F FOR VTER/P AND VTEK/P
+302°F FOR VTEL/P AND VTES/P

DIMENSIONS:

H = 4.33in (VTEK/P and VTER/P),
5.87in (VTEL/P and VTES/P)
N = 1.63in (VTEK/P and VTER/P)
3.17in (VTEL/P and VTES/P)
∅ = 1.05in

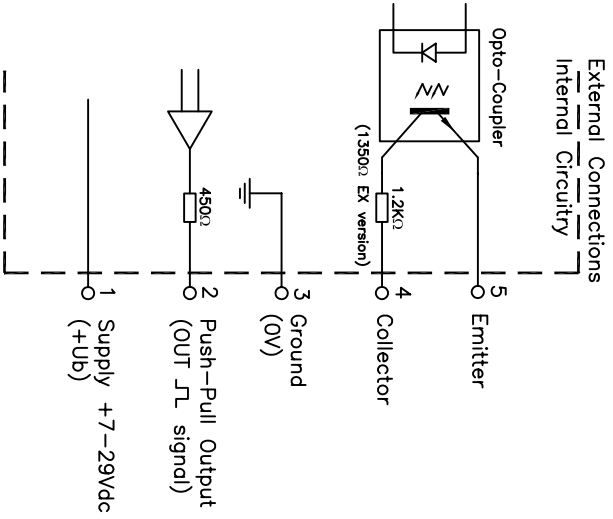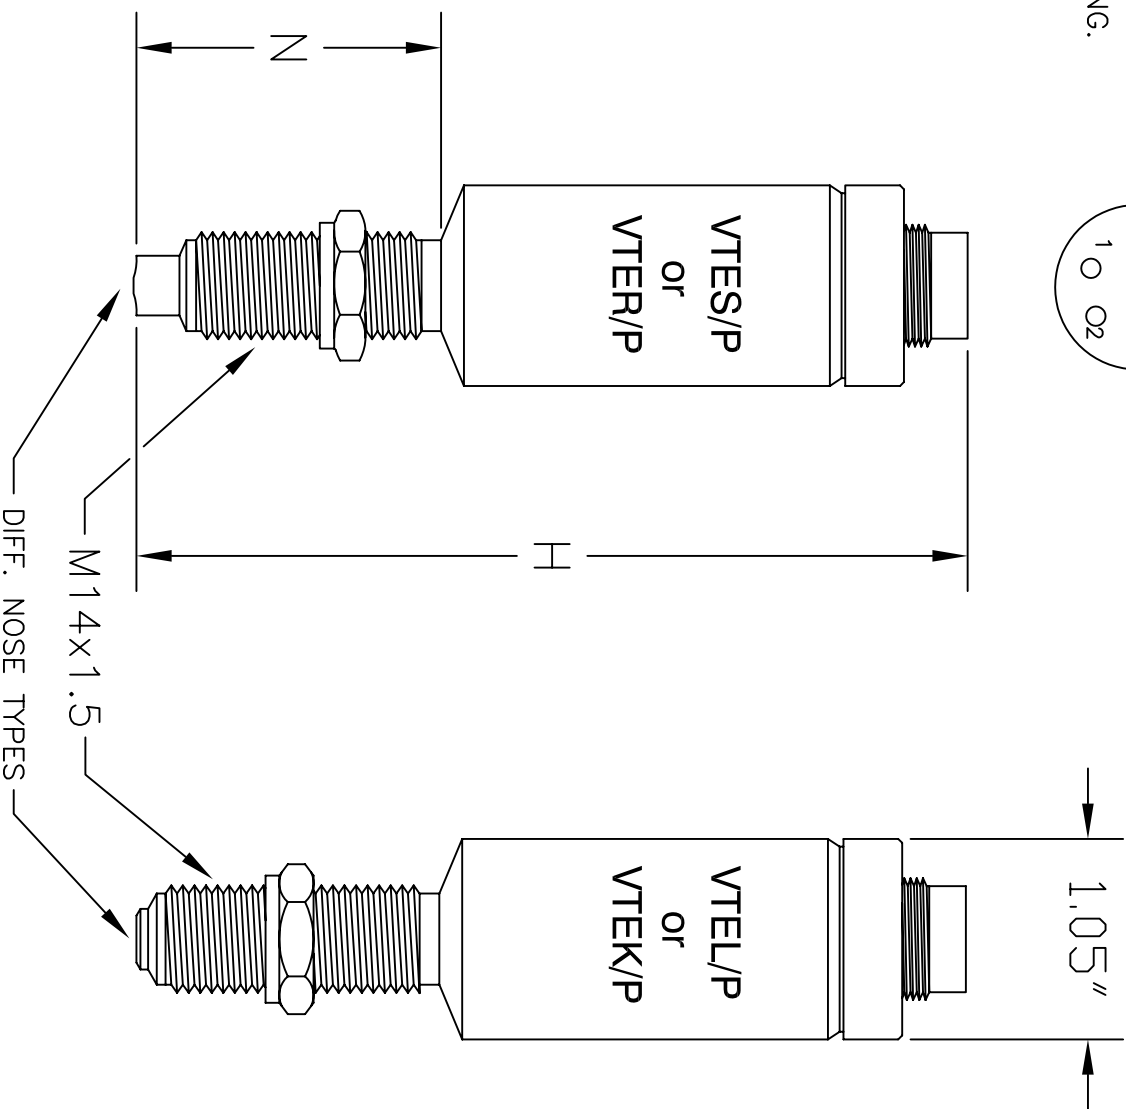

PURCHASED PART DRAWING

THIS PRINT, INCLUDING THE INFORMATION CONTAINED IN IT, IS THE PROPERTY OF AW-LAKE COMPANY. IT IS NOT TO BE REPRODUCED, COPIED, OR DISCLOSED OUTSIDE OF AW-LAKE COMPANY, EXCEPT UNDER PRIOR WRITTEN AGREEMENT. ANY MODIFICATIONS MADE TO OR COMMENTS WRITTEN ON THIS DRAWING BY UNAUTHORIZED PERSONNEL WILL VOID THIS DRAWING. ALL DIMENSIONS SHOWN ARE SUBJECT TO CHANGE WITHOUT NOTICE.



AW-LAKE COMPANY
A TASI GROUP COMPANY

8809 INDUSTRIAL DRIVE
FRANKSVILLE, WI 53126
TEL. # (262) 884-9800
FAX. # (262) 884-9810

TITLE: VTxx/P PICKUP SENSOR		PART NUMBER: —	
DRAWING NUMBER: VTER700C		DATE: 08-28-01	
REV: C	REV: C	DRAWN BY: SHANE WILSON	SCALE: NONE
CHECKED BY: C.H.	PAGE: 1	OF: 1	